

CEILING HEIGHT: N.A. WIRING DIAGRAM: 325623	MEDICAL GAS OUTLETS	
FASCIA COLOR	KEY STYLE: [ ] PURITAN BENNETT (QC)	
HPL MANUFACTURER: WILSONART COLOR: ANTIQUE WHITE 1572-60	[ ] CHEMETRON (QC)	
NURSE CALL PATIENT STATION	[ ] MEDAES (OHMEDA) (QC)	
MANUFACTURER: N.A. MODEL NUMBER: N.A.	[ ] DISS	
CODE BLUE	NOTE: MEDICAL GAS OUTLETS THAT ARE FURNISHED BY OTHERS MUST BE OF CONSOLE TYPE.	
MANUFACTURER: N.A. MODEL NUMBER: N.A.	PIPE SIZES	REGULATORY AGENCY APPROVAL
NURSE ASSIST	OXY 1/2" NOM.	U.L. LISTED
MANUFACTURER: N.A. MODEL NUMBER: N.A.	AIR 1/2" NOM.	OSHPD R-0138
	VAC 3/4" NOM.	ASTM B819

NOTE: CIRCUIT IDENTIFICATION (PANEL & CIRCUIT NUMBER) ON COVERPLATE OF POWER RECEPTACLES IF REQUIRED SHALL BE DONE IN THE FIELD BY OTHERS. FOR AN ADDITIONAL CHARGE, HOSPITAL SYSTEMS WILL ENGRAVE THE COVERPLATES WITH CIRCUIT I.D.

QTY. REQ'D: 1-UNIT


SERIAL NO. 9000-0000-01

ROOM NO.

LEGEND		
ITEM	DESCRIPTION	QTY
OXY	OXYGEN OUTLET	1
AIR	AIR OUTLET	1
VAC	VACUUM OUTLET	1
1	DUPLEX RECEPTACLE, RED	2
7	TIMER SWITCH, 60 MINUTES	1
12	FACEPLATE, NIGHT LIGHT (VENT)	1
67	VENT PLUG	2
68	VACUUM BOTTLE SLIDE, ADJ	1

GENERAL NOTES	
BASIC FRAME IS CONSTRUCTED OF DEEP ETCHED, CLEAR ANODIZED EXTRUDED ALUMINUM.	
FASCIA IS FINISHED WITH HIGH PRESSURE PLASTIC LAMINATED TO ALUMINUM BACKER. END CAPS ARE MOLDED GRAY PLASTIC, COLOR TO MATCH BASIC FRAME.	
ECLIPSE EQUIPMENT RAIL IS INTEGRAL TO EACH HORIZONTAL UNIT.	

NOTE: GAS OUTLETS ARE NOT INTENDED FOR MEDICAL USE.

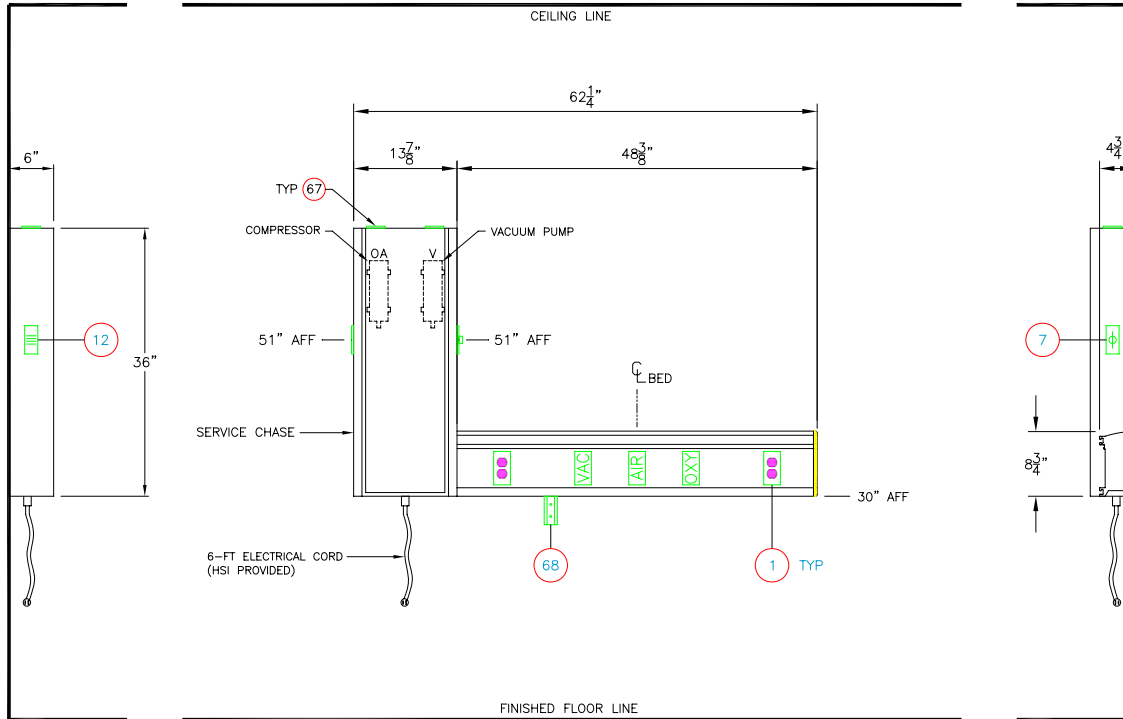

**HOSPITAL SYSTEMS**  
 750 Cordia Avenue, Pittsburg, CA 94965, USA  
 TEL: +1 925 427 7800 - FAX: +1 925 427 0800  
 [www.hospital-systems.com]

TITLE: COGENT TRAINING HEADWALL: HORIZONTAL  
 PROJECT: Hospital Systems, Inc., Pittsburg, California  
 9000

REVISION	DATE	BY	APP'D
1			
2			
3			
4			
5			

Drawn	BC
Date	06.12.07
Checked	
Scale	1/16"=1"
Part Number	1901822

THIS DOCUMENT WITH THE INFORMATION PRINTED HEREON ARE CONFIDENTIAL, PROPRIETARY PROPERTY OF HOSPITAL SYSTEMS, INC. AND ARE FURNISHED SOLELY FOR USE IN OBTAINING APPROVAL OF THE CONSTRUCTION DETAILS AND MATERIALS. NO PART OF THIS DOCUMENT MAY BE REPRODUCED, USED OR DISTRIBUTED EITHER IN WHOLE OR IN PART WITHOUT AUTHORIZATION FROM HOSPITAL SYSTEMS, INC.